


User Guide

CD81 TRIFic™

Exosome Detection System

Europium time-resolved immuno-
fluorescence assay for detection
of exosome antigens

Cat EX103

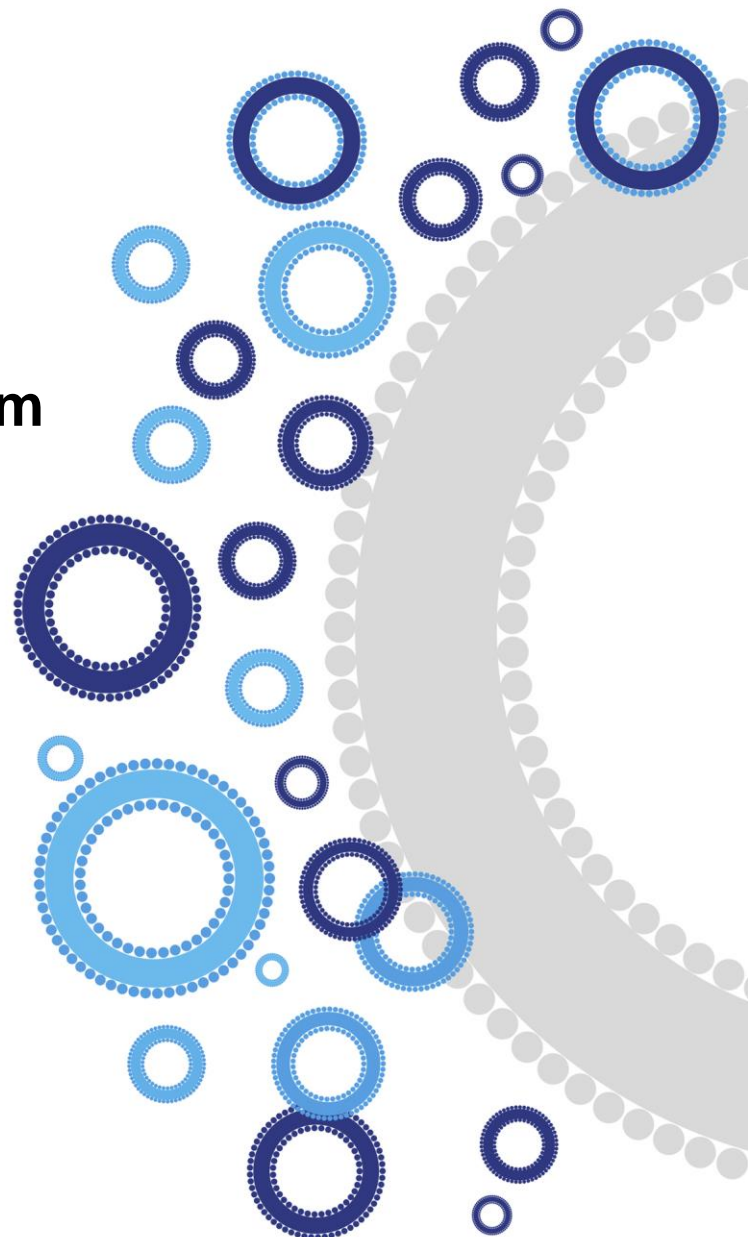

Contents

| | |
|--|----|
| Storage | 4 |
| Product components | 4 |
| Equipment and materials required but not supplied with this kit..... | 4 |
| Product information | 5 |
| Introduction and assay principle | 5 |
| General note..... | 6 |
| Reagent preparation | 6 |
| Technical positive control preparation..... | 6 |
| See example assay reading on page 9. | 7 |
| Protocol..... | 7 |
| Coat the wells with CD81 capture antibody | 7 |
| Add the sample | 8 |
| Add the europium-labeled CD81 detection antibody | 8 |
| Signal enhancement and reading..... | 8 |
| Technical positive control example | 9 |
| Related products..... | 9 |
| Exo-spin™ purification kit..... | 9 |
| ExoFLARE™ tracking assay | 10 |
| NTA size profiling service | 10 |
| Purchaser Notification..... | 11 |

CD81 TRIFic™

Exosome Detection System

Storage

- Store technical positive control at -80°C immediately upon receipt.
- Store all other components at 4°C.
- The kit has a shelf life of at least three months from receipt.

Product components

- 1 x Streptavidin-coated 96-well plate (8-well strip format)
- 1 x Technical positive control (100 µg/ml in PBS), 25 µg
N.B. The technical positive control is shipped on dry ice in a separate box
- 1 x Eu-labeled CD81 mAb (in 40 µl TSA buffer, 0.1% BSA), 2.75 µg
- 1 x Biotinylated CD81 mAb (in 22 µl PBS 7.4 pH, 15 mM NaN₃), 22 µg
The CD81 antibody used in the kit is human specific
- 1 x Assay buffer, 22 ml
- 1 x Europium fluorescence intensifier (EFI Solution), 11 ml
- 1 x 25x Wash buffer, 20 ml
- 1 x User Guide

Equipment and materials required but not supplied with this kit

- Time-resolved fluorescence microplate reader
- Automatic plate washer
- Plate shaker
- Pipettes for dispensing reagents
- Multichannel micropipette reservoir
- Distilled / Milli-Q water
- Phosphate buffered saline (PBS)


Product information

Introduction and assay principle

In the TRIFic™ exosome assay, the same antibody is used for binding of target to the assay plate and for detection. The assay consists of a monoclonal antibody (labeled with biotin) bound to a streptavidin-coated plate which captures protein present on the surface of exosomes (Figure 1). Subsequently, an identical monoclonal antibody (labeled with europium) is used for detection. Because the capture and detection antibody are identical, they require two linked copies of the same epitope for a signal to be detected. Exosomes provide an ideal structure to link CD81 molecules and allow detection of CD81 in this assay. Exosomes typically have multiple copies of CD81 facing towards the attachment surface and additional CD81 molecules available for detection. Any non-specific binding of capture and detection antibodies is unlikely to generate a signal. Using a europium fluorophore (see below) provides high levels of sensitivity for the assay, which is able to detect small changes in the abundance of the target CD81 protein even within unpurified complex biological samples, such as blood plasma and cerebral spinal fluid.

Fluorophores are chemical substances that emit light following excitation by light or other electromagnetic radiation. The emission of light from a fluorophore is maximal immediately following excitation and decays over a period of time. Time-resolved fluorimetry uses fluorophores which have long decay periods. For such fluorophores, measurement of emitted light can be performed when the excitation light is no longer present, thus increasing sensitivity.

Europium is a fluorophore which produces an extended emission decay and has a wide Stokes shift with maximal excitation at 340 nm and peak emission at 615 nm. TRIFic™ assays are time-resolved immunofluorescence assays which utilize europium and have been developed to measure the abundance of CD81 protein specifically associated with exosomes in biological fluids including urine, saliva, cell culture medium, cerebral spinal fluid and blood plasma.

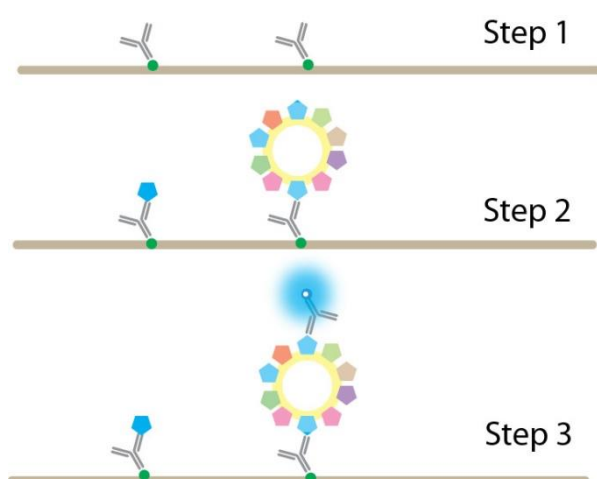

Step 1. Biotinylated antibody is bound to streptavidin-coated assay plates.

Step 2. Biological samples are added. Exosomes and any free antigen are captured by the antibody.

Step 3. Europium-labeled antibody is added and binds specifically to exosome antigen. The epitopes of bound monomers are already occupied and not detected. Samples are read in a time-resolved fluorescence plate reader.

Figure 1. Protocol overview

General note

The technical positive control provided with the kit can be used to verify that adequate technical and handling procedures have been conducted and a signal can be detected at the end of the protocol. The provided technical positive control cannot be used to generate a quantification curve for directly quantifying exosomes. Extracellular vesicles of different origin have different CD81 prevalence on their surface.

If absolute quantification is required, an internal quantification curve can be obtained for each population of exosomes studied by correlating CD81 TRIFic™ signal intensity with Nanoparticle Tracking Analysis (NTA) measurements at different concentrations of purified exosomes.

Reagent preparation

- **Preparation of the wash buffer:** Dilute the wash buffer concentrate 25x in Milli-Q water (20 ml concentrate in 500 ml Milli-Q water). The diluted solution may then be stored at room temperature.
- **Preparation of the biotin CD81 in assay buffer:** [Dilutions should be made on the day the assay is performed]. Briefly centrifuge the vial containing the antibody to gather all the liquid at the base of the vial. Prepare a ~2 ng/μl working solution of biotinylated Ab by diluting 22 μl (22 μg) in 11 ml of assay buffer.
- **Preparation of the europium CD81 in assay buffer:** [Dilutions should be made on the day the assay is performed]. Briefly centrifuge the vial containing the antibody to gather all the liquid at the base of the vial. Prepare a ~0.25 ng/μl working solution of Eu-labeled CD81 mAb by diluting 40 μl (2.75 μg) in 11 ml of assay buffer.

Technical positive control preparation

1. 25 μg of exosomes have been purified from cell culture and their total protein concentration determined by Bradford assay. The 25 μg of exosomes are provided in 250 μl PBS, at a concentration of **100 μg/ml**.
2. Prepare 7 microcentrifuge tubes, each with 125 μl of PBS.
3. Prepare 8 serial dilutions as shown in the table below. Ensure that samples are properly mixed in each tube.

We recommend beginning with a concentration of 100 μg/ml, as this will ensure that the most diluted sample is within the limit of detection of the assay.

Table 1. Positive control preparation

| Technical positive control # | Exosomes | Diluted in PBS (μl) | Exosome concentration (125 μl solution) |
|------------------------------|---|----------------------------------|--|
| 1 | 25 μg (in 250 μl PBS) | 250 | 100 $\mu\text{g}/\text{ml}$ |
| 2 | 125 μl of Tube #1 | 125 | 50 $\mu\text{g}/\text{ml}$ |
| 3 | 125 μl of Tube #2 | 125 | 25 $\mu\text{g}/\text{ml}$ |
| 4 | 125 μl of Tube #3 | 125 | 12.5 $\mu\text{g}/\text{ml}$ |
| 5 | 125 μl of Tube #4 | 125 | 6.3 $\mu\text{g}/\text{ml}$ |
| 6 | 125 μl of Tube #5 | 125 | 3.1 $\mu\text{g}/\text{ml}$ |
| 7 | 125 μl of Tube #6 | 125 | 1.6 $\mu\text{g}/\text{ml}$ |
| 8 | 125 μl of Tube #7 | 125 | 0.8 $\mu\text{g}/\text{ml}$ |

See example assay reading on page 9.

Protocol

Coat the wells with CD81 capture antibody

1. Add 100 μl of the freshly prepared dilute solution (2 $\text{ng}/\mu\text{l}$) of biotin-CD81 antibody (prepared as described above) to each well.
2. Incubate the plate for 1 hour at room temperature on a plate shaker at 750 RPM.
3. Wash the plate using an automatic plate washer. Wash each well three times using 250 μl wash buffer for each cycle.
4. Remove the remaining wash buffer.

Add the sample

5. Clear cells and cellular debris from test samples by centrifuging at 3,000 x g for 20 minutes.
6. Transfer 100 µl of the test sample supernatant to each well. Use 100 µl of PBS instead of sample in order to generate a blank reading.
7. Incubate the plate for 1 hour at room temperature on the plate shaker at 750 RPM.
8. Wash the plate using an automatic plate washer. Wash each well three times using 250 µl wash buffer each time.
9. Carefully aspirate the remaining wash buffer.

Add the europium-labeled CD81 detection antibody

10. Add 100 µl per well of the freshly prepared Eu-labeled CD81 antibody dilution (prepared as described above).
11. Incubate the plate for 1 hour at room temperature on the plate shaker at 750 RPM.
12. Wash the plate using an automatic plate washer. Wash each well three times using 250 µl wash buffer each time.
13. Carefully aspirate the remaining wash buffer.

Signal enhancement and reading

14. Add 100 µl of EFI solution to each well.
15. Incubate the plate for 15 minutes at room temperature on the plate shaker at 750 RPM.
16. Measure fluorescence on a time-resolved fluorescence microplate reader as shown on the table below. **Measurements should be performed in triplicate. Before taking the readings, make sure that the plate reader is set to read the fluorescence at the bottom of the plate.**

Table 2. Instrument settings

| Optic settings | Time resolved fluorescence (TRF) | |
|------------------|----------------------------------|--|
| | Filters | Excitation: 340 nm Emission: 615 nm |
| General settings | Number of flashes | 200 with flash lamp |
| | Settling time | 0.3 s |
| | Integration start/lag time | 200 µs |
| | Integration time | 400 µs |

Technical positive control example

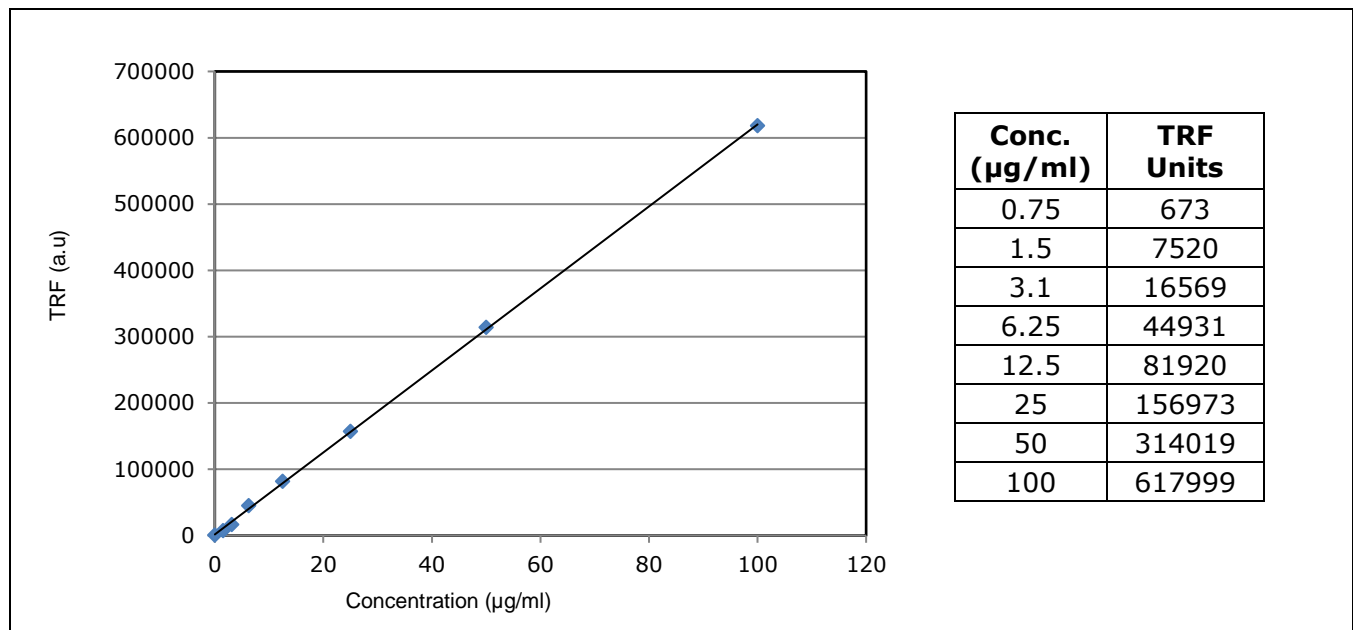


Figure 2. Example readings obtained using the TRIFic™ exosome assay with the provided technical control sample (exosomes purified from cell culture). Note the linearity of response over a wide range of concentrations.

Related products

| Related products | Product description | Product code |
|---|--|--|
| Exosome purification | Exo-spin™ purification kit | EX01, EX02, EX03, EX04, EX05 |
| Exosome tracking | ExoFLARE™ tracking assay | EX301, EX302, EX303, EX304, EX305, EX306 |
| Nanoparticle Tracking Analysis (NTA) size profiling service | ZetaView NTA Particle Analysis Service | ZV-1 and ZV-12 |

Exo-spin™ purification kit

The Exo-spin™ technology combines precipitation and size exclusion chromatography techniques, making it a superior method for exosome separation and concentration, allowing for high specificity and high recovery of exosomes. Exo-spin™ is available in 5 different configurations represented with catalogue codes EX01, EX02, EX03, EX04, and EX05; specifically designed and optimized for different sample types and downstream applications.

ExoFLARE™ tracking assay

ExoFLARE™ utilizes a combination of a FLARE (FLuorescence Activating Response Element) protein tag together with a pro-fluorophore dye. Neither the protein nor dye exhibit fluorescence in isolation. However, when the protein binds to the dye, it causes a change in structure which results in fluorescence. The dye and protein form an unstable bond with a continuous turnover of the dye, resulting in sustained fluorescence without the levels of photo-bleaching associated with fluorescent proteins (i.e. GFP). This enables ExoFLARE™ to be monitored for extensive periods to allow tracking of dye movement.

NTA size profiling service

Exosome characterization service for analysis of particle size and particle concentration using the ZetaView instrument from Particle Metrix.

Purchaser Notification

Limited warranty Cell Guidance Systems and/or its affiliate(s) warrant their products as set forth in the Terms of Sale found on the Cell Guidance Systems web site at www.cellgs.com/Pages/Terms_and_Conditions.html

If you have any questions, please contact Cell Guidance Systems.

This product incorporates licensed technologies. The purchase of this product conveys to the purchaser the limited, nontransferable right to use the purchased amount of the product only to perform internal research for the sole benefit of the purchaser. No right to resell this product or any of its components is conveyed. This product is for internal research purposes only and is not for use in commercial services of any kind, including, without limitation, reporting the results of purchaser's activities for a fee or other form of consideration. For information on obtaining additional rights, please contact info@cellgs.com.

CELL GUIDANCE SYSTEMS AND/OR ITS AFFILIATE(S) DISCLAIM ALL WARRANTIES WITH RESPECT TO THIS DOCUMENT, EXPRESSED OR IMPLIED, INCLUDING BUT NOT LIMITED TO THOSE OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE, OR NON-INFRINGEMENT. TO THE EXTENT ALLOWED BY LAW, IN NO EVENT SHALL CELL GUIDANCE SYSTEMS AND/OR ITS AFFILIATE(S) BE LIABLE, WHETHER IN CONTRACT, TORT, WARRANTY, OR UNDER ANY STATUTE OR ON ANY OTHER BASIS FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING BUT NOT LIMITED TO THE USE THEREOF.

Cell Guidance Systems' reagents and services enable control, manipulation and monitoring of the cell, both *in vitro* and *in vivo*

Growth Factors

- Recombinant
- Sustained Release

Exosomes

- Purification
- Detection
- Tracking
- NTA Service

Small Molecules

Cell Counting Reagent

Matrix Proteins

Cell Culture Media

- Pluripotent Stem Cells
- Photostable
- *In Vitro* Blastocyst Culture
- ETS-embryo Culture
- Custom Manufacturing Service

Gene Knock-Up System

Cytogenetics Analysis



General info@cellgs.com
Technical Enquiries tech@cellgs.com
Quotes quotes@cellgs.com
Orders order@cellgs.com

www.cellgs.com

EUROPE
Cell Guidance Systems Ltd
Maia Building
Babraham Bioscience Campus
Cambridge
CB22 3AT
United Kingdom
T +44 (0) 1223 967316
F +44 (0) 1223 750186

USA
Cell Guidance Systems LLC
Helix Center
1100 Corporate Square Drive
St. Louis
MO 63132
USA
T 760 450 4304
F 314 485 5424